

## **TETRODOTOXIN SENSITIVE ELISA**

*5191TTXSENS[1]02.22*

A competitive enzyme immunoassay  
for the quantitative analysis of tetrodotoxin in  
fish and shellfish

# EUROPROXIMA TETRODOTOXIN SENSITIVE ELISA

## A competitive enzyme immunoassay for the quantitative analysis of tetrodotoxin in fish and shellfish

### TABLE OF CONTENTS

	PAGE:
Brief Information .....	2
1. Introduction .....	2
2. Principle of the Tetrodotoxin Sensitive ELISA.....	2
3. Specificity and Sensitivity .....	3
4. Handling and Storage .....	3
5. Kit contents .....	4
6. Equipment and materials required but not provided...	5
7. Precautions .....	5
8. Sample preparations .....	6
9. Preparation of reagents .....	6
10. Assay Procedure .....	7
11. Interpretation of results .....	9
12. Literature.....	10
13. Ordering information .....	10
14. Revision History .....	10

The quality management system of R-Biopharm Nederland B.V. is  
ISO 9001:2015 certified

## **BRIEF INFORMATION**

The Tetrodotoxin Sensitive (TTXSENS) ELISA is a competitive enzyme immunoassay for the quantitative detection of tetrodotoxin in fish and shellfish. With this ELISA-kit 96 analyses can be performed. Samples and standards are measured in duplicate which means that a total of 40 samples can be analysed. The TTXSENS ELISA contains all reagents needed to perform the test.

## **1. INTRODUCTION**

Tetrodotoxin (TTX) and its analogues belong to a group of neurotoxins that are produced by various marine bacteria. The toxin can accumulate in certain species of fish, different marine bivalves (clams, oysters and mussels) and gastropods. Due to the worldwide increase in water temperature TTX has appeared also in the European waters. TTX has been recently detected in seafood harvested in the United Kingdom, Portugal, Spain, Greece and the Netherlands. The ingestion of contaminated seafood can have fatal consequences. On the cellular level TTX causes blockage of voltage-gated sodium channels that leads to alteration of neuronal functions and muscle paralysis. Death can occur due to heart or respiratory failure. The majority of the poisoning cases have been caused by the consumption of pufferfish contaminated with TTX in Japan, where a limit of 2000 µg/kg was set for fish. As for now there are no maximum limits for TTX in the European Union. According to the recent European Food Safety Authority Scientific Opinion the concentration of TTX and its analogues of 44 µg/kg of shellfish meat should not result in adverse effects in humans.

## **2. PRINCIPLE OF THE TETRODOTOXIN Sensitive ELISA**

The microtiter plate based TTXSENS ELISA consists of one plate (12 strips, 8 wells each) pre-coated with TTX-protein conjugate. In the first step of the assay mouse monoclonal antibody and standards or samples are added to the pre-coated wells. TTX present in the standard solutions or in the samples and TTX immobilized on the surface of the wells compete for binding to the antibody (competitive enzyme immunoassay). After incubation, non-bound reagents are removed in a washing step. The bound antibody TTX complex is detected by addition of horseradish peroxidase (HRP) labeled anti-mouse antibody. After a washing step, the amount of bound complex is visualized by addition of enzyme/chromogen (hydrogen peroxide/tetramethylbenzidine, TMB). During the incubation the colourless chromogen is converted by the enzyme into a blue reaction product. The colour intensity is inversely proportional to the amount of TTX in the sample/standard, i.e. the more TTX present in the standard solution or sample, the less colour is developed. The colour development is stopped by addition of sulfuric acid. The intensity of yellow colour formed is measured photometrically at 450 nm.

### 3. SPECIFICITY AND SENSITIVITY

For this TTXSENS ELISA a specific antibody is used, obtained by immunisation of mice with a TTX protein conjugate. The cross-reactivity profile of the antibody (as tested in buffer) is:

Tetrodotoxin	100%
Okadaic acid	<0.1%
Saxitoxin	<0.1%
Domoic acid	<0.1%

The cross-reactivities are determined in a buffer system. The reported values may be different in samples due to matrix effects.

The test cannot discriminate between analytes and cross-reactive substances.

The limit of detection (LOD) and the detection capability (CC $\beta$ ) are determined under optimal conditions. Cut-off criteria need critical consideration.

Matrix	Procedure	LOD ( $\mu\text{g/kg}$ )	CC $\beta$ ( $\mu\text{g/kg}$ )
Fish and shellfish	8.1	1.4	6.0

If the sample is found to be non-compliant, the results shall be verified by re-analysis of the sample using a confirmatory method.

### 4. HANDLING AND STORAGE

- Kit and kit components should be stored at 2°C to 8°C in a dark place. For repeated use store kit components as specified under chapter 9.
- After the expiry date of the kit and/or components has passed, no further quality guarantee is valid.
- Bring all kit components including the microtiter plate to ambient (room) temperature before use.
- Dilute the kit components immediately before use, but after the components are brought to ambient temperature.
- Avoid condensation in the wells of the plate. Bring the sealed plate to ambient temperature before opening the plate sealing.
- The substrate chromogen solution can be stored in a refrigerator (2°C to 8°C) until the expiry date stated on the label.
- Exposure of the chromogen solution to light should be avoided.

Degeneration of the reagents may have occurred when the following phenomena are observed:


- A blue colouring of the chromogen solution before transferring it into the wells.
- A weak or no colour reaction in the zero standard wells (E450nm < 0.8).

## 5. KIT CONTENTS

### Manual

One sealed (96-wells) microtiter plate (12 strips, 8 wells each), coated with TTX-protein conjugate. Ready-to-use.

Position of the reagents in the kit. For preparation of the reagents see Chapter 9.

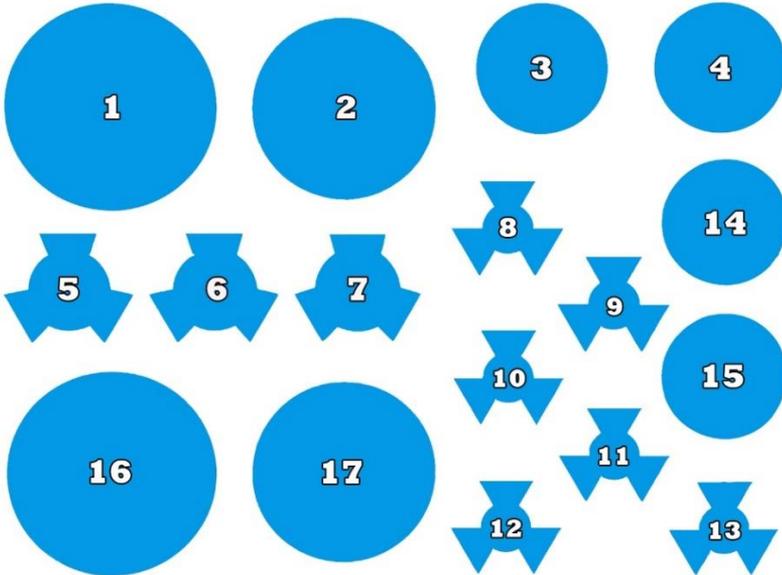

1. **Dilution buffer** (40 ml, 4x concentrated)
2. **Rinsing buffer** (30 ml, 20x concentrated)
3. **Substrate solution** (12 ml, ready-to-use)
4. **Stop solution** (12 ml, ready-to-use)
5. **Standard** (10 ng/ml, lyophilized)
6. **Standard** (10 ng/ml, lyophilized)
7. **Standard** (10 ng/ml, lyophilized)
8. **Conjugate** (150  $\mu$ l, 100x concentrated)
9. **Antibody** (100  $\mu$ l, 100x concentrated)
10. Not in use
11. Not in use
12. Not in use
13. Not in use
14. Not in use
15. Not in use
16. Not in use
17. **Extraction buffer** (20 ml, 10x concentrated)

## 6. EQUIPMENT AND MATERIALS REQUIRED BUT NOT PROVIDED

- Scales and weighing vessels
- Gloves
- Fume hood
- Homogeniser
- Vortex mixer
- Centrifuge (4300 x g)
- Automated microplate washer or 8-channel micropipette 100 – 300 µl
- Microtiter plate shaker
- Microtiter plate reader with 450 nm filter
- Micropipettes 20 – 200 µl, 100 – 1000 µl
- Multipipette with 2.5 ml combitips
- Aluminium foil or parafilm
- Deionised or distilled water

## 7. PRECAUTIONS

- This kit may contain hazardous substances. For hazard notes please refer to the appropriate safety data sheets (SDS).
- Avoid contact of all biological materials with skin and mucous membranes.
- Do not pipette by mouth.
- Do not eat, drink, smoke, store or prepare foods, or apply cosmetics within the designated work area.
- Do not use components past expiration date and do not use components from different lots.
- Each well is ultimately used as an optical cuvette. Therefore, do not touch the under surface of the wells, prevent damage and dirt.
- All components should be completely dissolved before use. Take special attention to the substrate and rinsing buffer, which crystallize at +4°C.
- Optimal results will be obtained by strict adherence to this protocol. Careful pipetting and washing throughout this procedure are necessary to maintain good precision and accuracy.

R-Biopharm Nederland makes no warranty of any kind, either expressed or implied, except that the materials from which its products are made are of standard quality. There is no warranty of merchantability of this product, or of the fitness of the product for any purpose. R-Biopharm Nederland shall not be liable for any damages, including special or consequential damage, or expense arising directly or indirectly from the use of this product.

## 8. SAMPLE PREPARATION

### 8.1 Fish and shellfish

- Add 3 ml of the diluted extraction buffer (see chapter 9) to 1 g of the homogenised sample
- Vortex shortly and then mix head over head for 5 minutes
- Centrifuge 5 minutes at 4000 x g (20-25°C)
- Dilute sample supernatant 3 times with the dilution buffer (e.g., add 100 µl of the supernatant to 200 µl of the dilution buffer)
- Mix well and use 50 µl directly in the ELISA.

## 9. PREPARATION OF REAGENTS

Before beginning the test, the reagents should be brought up to room temperature. Any reagents not used should be put back into storage immediately at +2°C to +8°C. Prepare reagents freshly before use.

### Microtiter plate

Return unused strips into the resealable bag with desiccant and store at +2°C to +8°C for use in subsequent assays. Retain also the strip holder.

### Rinsing buffer

The rinsing buffer is delivered 20 times concentrated. Prepare dilutions freshly before use. For each strip 20 ml of diluted rinsing buffer is used (1 ml concentrated rinsing buffer + 19 ml distilled water).

### Dilution buffer

The dilution buffer is 4 times concentrated. Mix well and dilute 4 times in deionised water, for example add 20 ml of concentrated buffer to 60 ml of water and mix well. The diluted buffer can be stored in a refrigerator (+2°C to +8°C) for up to 1 month.

### Conjugate solution

The conjugate is delivered 100x concentrated. Spin down the conjugate in the vial by a short centrifugation step (1 min., 1000 x g). Add 20 µl of the concentrated conjugate solution to 1980 µl of the dilution buffer. Per 2 x 8 wells 1.6 ml of diluted conjugate is required. Store unused concentrated conjugate at +2°C to +8°C.

### Antibody

The antibody is delivered 100x concentrated. Spin down the antibody in the vial by a short centrifugation step (1 minute, 1000 x g). Add 10 µl of the concentrated antibody solution to 990 µl of the dilution buffer. Per 2 x 8 wells 800 µl of diluted antibody is required. Store unused concentrated antibody at +2°C to +8°C.

### Extraction buffer

The extraction buffer is 10x concentrated. Mix well and dilute 10 times in deionized water, for example add 5 ml of concentrated buffer to 45 ml of water. The diluted

extraction buffer can be stored in a refrigerator (+2°C to +8°C) for up to 1 month.

#### Substrate/chromogen solution

The substrate/chromogen solution (ready-to-use) tends to precipitate at +4°C. Take care that this vial is at room temperature when used (keep in the dark) and mix the content before pipetting into the wells.

#### Standards

Prepare a dilution range of TTX standards. Add 2 ml of the dilution buffer to the TTX standard and mix. This solution contains 10 ng of TTX per ml. Pipette 0.25 ml of this solution into a clean tube and add 0.25 ml of the dilution buffer. Continue to make a dilution range of 10, 5, 2.5, 1.25, 0.625 and 0.3125 ng/ml.

## **10. ASSAY PROCEDURE**

### Rinsing protocol

In ELISAs, between each immunological incubation step, unbound components have to be removed efficiently. This is reached by appropriate rinsing. It should be clear that each rinsing procedure must be carried out with care to guarantee good inter- and intra-assay results.

Manual rinsing or rinsing with automatic plate wash equipment can be performed as follows:

### Manual rinsing

1. Empty the contents of each well by turning the microtiter plate upside down followed by a firm short vertical movement.
2. Fill all the wells to the rims (300 µl) with rinsing solution.
3. This rinsing cycle (1 and 2) should be carried out 3 times.
4. Turn the plate upside down and empty the wells by a firm short vertical movement.
5. Place the inverted plate on absorbent paper towels and tap the plate firmly to remove residual washing solution in the wells.
6. Take care that none of the wells dry out before the next reagent is dispensed.

### Rinsing with automatic microtiter plate wash equipment

When using automatic plate wash equipment, check that all wells can be aspirated completely, that the rinsing solution is nicely dispensed reaching the rim of each well during each rinsing cycle. The washer should be programmed to execute three rinsing cycles.

### Assay Protocol

1. Prepare samples according to Chapter 8 and prepare reagents according to Chapter 9.

2. Pipette 100  $\mu$ l of the zero standard in duplicate (wells H1, H2, blank).  
Pipette 50  $\mu$ l of the zero standard in duplicate (wells A1, A2, maximal signal).  
Pipette 50  $\mu$ l of each of the standard solutions in duplicate (wells B1,2 to G1,2 i.e. 10, 5, 2.5, 1.25, 0.625, 0.3125 ng/ml)
3. Pipette 50  $\mu$ l of each sample solution in duplicate into the remaining wells of the microtiter plate.
4. Pipette 50  $\mu$ l of antibody into all wells, except the blank H1 and H2.
5. Seal the microtiter plate and shake the plate for a few seconds on a microtiter plate shaker.
6. Incubate for 30 minutes in the dark at room temperature (20-25°C).
7. Discard the solution from the microtiter plate and wash 3 times with rinsing buffer.
8. Pipette 100  $\mu$ l of conjugate into each well, except H1 and H2.
9. Seal the microtiter plate and shake the plate for a few seconds on a microtiter plate shaker.
10. Incubate for 15 minutes in the dark at room temperature (20-25°C).
11. Discard the solution from the microtiter plate and wash 3 times with rinsing buffer.
12. Pipette 100  $\mu$ l of substrate solution into each well.
13. Incubate 15 minutes at room temperature (20°C - 25°C).
14. Add 100  $\mu$ l of stop solution into each well.
15. Read the absorbance values immediately at 450 nm.

## 11. INTERPRETATION OF RESULTS

Subtract the mean optical density (O.D.) of the wells H1 and H2 from the individual O.D. of the wells containing the standards and the samples.

The O.D. values of the six standards and the samples (mean values of the duplicates) are divided by the mean O.D. value of the zero standard (wells B1 and B2) and multiplied by 100. The zero standard is thus made equal to 100% (maximal absorbance) and the other O.D. values are quoted in percentages of the maximal absorbance.


$$\frac{O.D. \text{ standard (or sample)}}{O.D. \text{ zero standard}} \times 100 = \text{percentage maximal absorbance}$$

### Calibration curve:

The values (percentage maximal absorbance) calculated for the standards are plotted (on the Y-axis) versus the TTX concentration (ng/ml) on a logarithmic X-axis.

### Alternative for calibration curve:

The value of absorption (logit) calculation of the standards are plotted on Y-axis versus the analyte equivalent concentration on a logarithmic X-axis

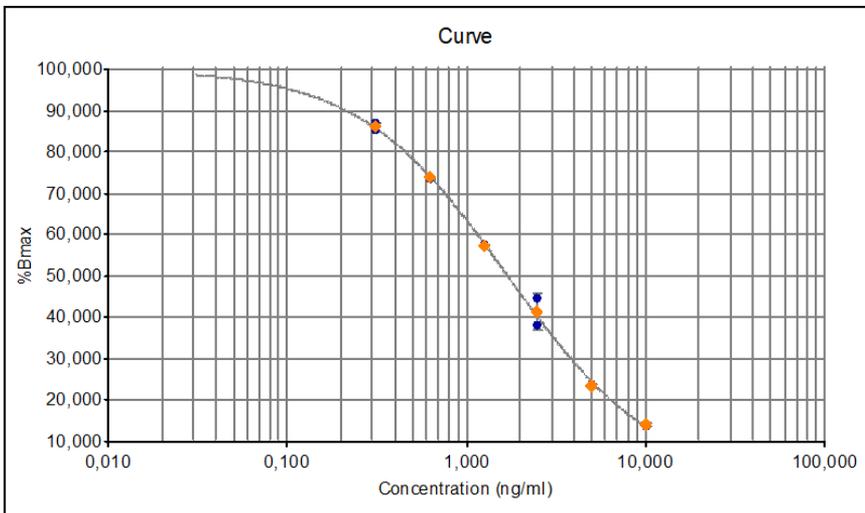

**Figure 1 : Example of a calibration curve**

### Calculation factors

To obtain the TTX concentration in a sample ( $\mu\text{g}/\text{kg}$ ), the TTX concentration read from the calibration curve has to be multiplied by a factor 12. This factor is applicable for the sample preparation method for fish and shellfish.

## **12. LITERATURE**

European Food Safety Authority (EFSA). Risks for public health related to the presence of tetrodotoxin (TTX) and TTX analogues in marine bivalves and gastropods. *EFSA Journal* 2017, 15(4):4752.

Lago J., Rodríguez L.P., Blanco L., Vieites J.M. and Cabado A.G. Tetrodotoxin, an extremely potent marine neurotoxin: distribution, toxicity, origin and therapeutical uses. *Mar. Drugs* 2015, 13, 6384-6406.

## **13. ORDERING INFORMATION**

For ordering the Tetrodotoxin ELISA, please use catalogue code 5191TTXSENS Tetrodotoxin Sensitive ELISA.

## **14. REVISION HISTORY**

Not applicable